

REC'D 17 FEB 2005

IB/05/050447



WIPO  
Europäisches  
Patentamt

PCT  
European  
Patent Office

Office européen  
des brevets

Bescheinigung

Certificate

Attestation

Die angehefteten Unterlagen stimmen mit der ursprünglich eingereichten Fassung der auf dem nächsten Blatt bezeichneten europäischen Patentanmeldung überein.

The attached documents are exact copies of the European patent application described on the following page, as originally filed.

Les documents fixés à cette attestation sont conformes à la version initialement déposée de la demande de brevet européen spécifiée à la page suivante.

Patentanmeldung Nr. Patent application No. Demande de brevet n°

04100475.5 ✓

**PRIORITY  
DOCUMENT**  
SUBMITTED OR TRANSMITTED IN  
COMPLIANCE WITH RULE 17.1(a) OR (b)

Der Präsident des Europäischen Patentamts;  
Im Auftrag

For the President of the European Patent Office

Le Président de l'Office européen des brevets  
p.o.

R C van Dijk





Anmeldung Nr:  
Application no.: 04100475.5 ✓  
Demande no:

Anmeldetag:  
Date of filing: 09.02.04 ✓  
Date de dépôt:

Anmelder/Applicant(s)/Demandeur(s):

Koninklijke Philips Electronics N.V.  
Groenewoudseweg 1  
5621 BA Eindhoven  
PAYS-BAS

Bezeichnung der Erfindung/Title of the invention/Titre de l'invention:  
(Falls die Bezeichnung der Erfindung nicht angegeben ist, siehe Beschreibung.  
If no title is shown please refer to the description.  
Si aucun titre n'est indiqué se référer à la description.)

An RF coil system for an MRI system with a fixed and a moving part

In Anspruch genommene Priorität(en) / Priority(ies) claimed /Priorité(s)  
revendiquée(s)  
Staat/Tag/Aktenzeichen/State/Date/File no./Pays/Date/Numéro de dépôt:

Internationale Patentklassifikation/International Patent Classification/  
Classification internationale des brevets:

G01R33/20

Am Anmeldetag benannte Vertragsstaaten/Contracting states designated at date of  
filing/Etats contractants désignées lors du dépôt:

AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IT LU MC NL  
PT RO SE SI SK TR LI



An RF coil system for an MRI system with a fixed and a moving part

The present invention relates to an RF system for a magnetic resonance imaging device, comprising an RF transmitter coil subsystem and an RF receiver coil subsystem.

5 The present invention also relates to a magnetic resonance imaging device, comprising a main magnet system, a gradient coil system, an RF system and a signal processing system, said RF system comprising an RF transmitter coil subsystem and an RF receiver coil subsystem.

10 The basic components of a magnetic resonance imaging (MRI) device are the main magnet system, the gradient coil system, the RF system and the signal processing system. The main magnet system typically comprises a bore hole enabling the entry of an object to be analyzed by the MRI device, and generates a strong uniform static field for polarization of nuclear spins in the object to be analyzed. The gradient coil system is designed to produce time-varying magnetic fields of controlled spatial non-uniformity. The RF system mainly consists of an RF transmitter coil subsystem and an RF receiver coil  
15 subsystem, wherein the RF transmitter coil subsystem is capable of generating a rotating magnetic field for excitation of nuclear spin resonance in the object to be analyzed, and wherein the RF receiver coil subsystem converts a precessing magnetization of spinning nuclei into electrical signals. The signal processing system generates images on basis of the electrical signals. The present invention is related to the RF system of such an MRI device,  
20 especially to the RF receiver coil subsystem of such an RF system.

It should be noted, that MRI devices which comprise the above-mentioned bore hole within the main magnet system are also often called cylindrical (or closed) MRI devices. The present invention is not limited to such cylindrical MRI devices. The invention can also be used in non-cylindrical (or open) MRI devices typically comprising a C-arm with  
25 a cavity instead of the bore hole.

From prior art two types of RF systems or RF receiver coil subsystems are known. According to a first type of such an RF system, the entire RF receiver coil subsystem

is fixed to the object to be analyzed, preferably around said object. Such RF systems have the disadvantage that there are many cables and moving parts that may interfere with a comfortable position of the object to be analyzed. Such an RF system may also hamper the preparation of the object to be analyzed, because a lot of coils have to be placed around said object. Within the second type of RF systems or RF receiver coil systems, the entire RF receiver coil system is fixed to the main magnet system of the magnetic resonance imaging device. This type of RF systems have the disadvantage that the RF receiver coil subsystem is positioned with a larger distance from the object to be analyzed, thereby resulting in a lower signal-to-noise ratio. Reference is made to the prior art US 5,600,245 and US 2002/0138001 A1.

It is an object of the invention to provide an RF system of the kind mentioned in the opening paragraph and a magnetic resonance imaging device of the kind mentioned in the opening paragraph in which the disadvantages of the known RF system and of the known magnetic resonance imaging device are prevented as much as possible.

In order to achieve said object, an RF system in accordance with the invention is characterized in that the RF receiver coil subsystem comprises at least one first coil-like element and at least one second coil-like element, wherein the or each first coil-like element is assigned to a main magnet system of the magnetic resonance imaging device, and wherein the or each second coil-like element is assigned to an object to be analyzed by the magnetic resonance imaging device.

In order to achieve said object, a magnetic resonance imaging device in accordance with the invention is characterized in that the RF receiver coil subsystem comprises at least one first coil-like element and at least one second coil-like element, wherein the or each first coil-like element is assigned to the main magnet system, and wherein the or each second coil-like element is assigned to an object to be analyzed by the magnetic resonance imaging device.

An RF system in accordance with the invention and a magnetic resonance imaging device comprising such an RF system have different advantages over the MRI devices and RF systems known from prior art. Compared to an RF system for which all coils are attached to the object to be analyzed and for which all coils move with the object to be analyzed, there are advantages for the operator of the magnetic resonance imaging device and for the object to be analyzed. For the operator, it is much easier to set up the object to be

analyzed because of the fact, that only the second coil-like element has to be attached to the object and that fewer cables have to be connected to the MRI device. For the object to be analyzed, the comfort can be increased, because of the fact, that there are no coils positioned between the bed and the posterior part of the object. In addition, there is more space available in the examination space. Compared to a device where all parts of the RF receiver coil subsystem are fixed to the main magnet system, a higher signal-to-noise ratio can be achieved, because of the fact that the parts of the RF receiver coil subsystem are positioned closer to the object to be analyzed.

In accordance with a preferred embodiment of the invention the or each first coil-like element is positioned below, preferably directly below, a support or bed on which the object to be analyzed is placed. The or each first coil-like element is attached to the main magnet system of the magnetic resonance imaging device, in a way that a relative movement between said support or bed and the or each first coil-like element is possible.

In accordance with a further improved, preferred embodiment of the invention the or each second coil-like element is positioned above, preferably directly above, the object to be analyzed. The or each second coil-like element is attached to the object to be analyzed, in a way that the or each second coil-like element is moveable together with the object to be analyzed. The or each second coil-like element is moveable together with a support or bed on which the object to be analyzed is placed relative to the or each first coil-like element.

Embodiments of an RF system and a magnetic resonance imaging device in accordance with the invention will be described in the following with reference to the figs., wherein

Fig. 1 shows an MRI device according to the prior art;

Fig. 2 shows an MRI device including an RF system, namely an RF receiver coil subsystem, according to a first embodiment of the present invention; and

Fig. 3 shows an MRI device including an RF system, namely an RF receiver coil subsystem, according to a second embodiment of the present invention.

Figure 1 shows a magnetic resonance imaging (MRI) device 1 known from prior art which includes a main magnet system 2 for generating a steady magnetic field, and also several gradient coils providing a gradient coil system 3 for generating additional

magnetic fields having a gradient in the X, Y, Z directions. The X direction of the coordinate system shown corresponds to the direction of the steady magnetic field in the main magnet system 2 by convention. The X axis is an axis co-axial with the axis of an examination space of the main magnet system 2, whereby the Z axis is the vertical axis extending from the center of the magnetic field, and whereby the Y axis is the corresponding horizontal axis orthogonal to the X axis and the Z axis. The gradient coils of the gradient coil system 3 are fed by a power supply unit 4.

The magnetic resonance imaging (MRI) device 1 according to fig. 1 further includes an RF system 5 comprising an RF transmitter coil subsystem and an RF receiver coil subsystem. The RF transmitter coil subsystem serves to generate RF magnetic fields and is connected to an RF transmitter and modulator 6. The RF receiver coil subsystem is used to receive the magnetic resonance signal generated by the RF field in the object 7 to be examined, for example a human or animal body.

Furthermore, the main magnet system 2 encloses an examination space which is large enough to accommodate a part of the body 7 to be examined. The RF system 5, namely the RF receiver coil subsystem, is connected to a signal amplifier and demodulation unit 10 via a transmission/reception circuit 9.

The control unit 11 controls the RF transmitter and modulator 6 and the power supply unit 4 so as to generate special pulse sequences which contain RF pulses and gradients. The phase and amplitude obtained from the demodulation unit 10 are applied to a processing unit 12. The processing unit 12 processes the presented signal values so as to form an image by transformation. This image can be visualized, for example by means of a monitor 8.

According to the present invention, the magnetic resonance imaging (MRI) device 1 comprises an improved RF system, namely an improved RF receiver coil subsystem, which will be described below in greater detail. The present invention provides a new RF system for magnetic resonance imaging devices.

Fig. 2 shows a magnetic resonance imaging device 13 together with an object 14 to be analyzed in two different positions of said object 14. Fig. 2 shows a main magnet system 15 of the magnetic resonance imaging device 13 enclosing an examination space 16, whereby said examination space 16 is large enough to accommodate at least a part of the object 14 to be analyzed. The object 14 to be analyzed is positioned on a support or bed 17, whereby the support or bed 17 can be moved relative to the main magnet system 15, so that the object 14 to be analyzed can be inserted into the examination space 16 or removed from



said examination space 16. In the upper part of Fig. 1, the object 14 to be analyzed is nearly completely inserted in the examination space 16. In the lower part of fig. 1, the object 14 to be analyzed is nearly completely removed from the examination space 16.

5 In addition to the main magnet system 15 enclosing said examination space 16, the magnetic resonance imaging device 13 according to the present invention comprises also a gradient coil system and an RF system. In order to simplify the drawing of fig. 2, the gradient coil system is not shown in fig. 2. In addition, only the RF receiver coil subsystem 18 of the RF system is shown in fig. 2.

10 The RF receiver coil subsystem 18 according to the present invention comprises at least one first coil-like element 19 and at least one second coil-like element 20. The or each first coil-like element 19 is assigned to the main magnet system 15 of the magnetic resonance imaging device 13. The or each first coil-like element 19 may be designed as part of a built-in system body coil. The or each second coil-like element 20 is assigned to the object 14 to be analyzed by the magnetic resonance imaging device 13. Fig. 2  
15 shows only one first coil-like element 19 and one second coil like element 20. Each of these coil-like elements may comprise one or more loops.

According to the embodiment of fig. 2, the first coil-like element 19 of the RF receiver coil subsystem 18 is attached to the main magnet system 15 and positioned directly below the support or bed 17 on which the object to be analyzed is placed. The first coil-like  
20 element 19 of the RF receiver coil subsystem 18 is, according to the embodiment of fig. 2, fixedly attached to the main magnet system 15. This allows a movement of the support or bed 17 relative to the main magnet system 15 and relative to the first coil-like element 19.

The second coil-like element 20 of the RF receiver coil subsystem 18 is attached to the object 14 to be analyzed, namely directly above the object 14. The second  
25 coil-like element 20 is movable together with the support or bed 17 and therefore together with the object 14 to be analyzed relative to the main magnet system 15 and relative to the first coil-like element 18.

Within the embodiment shown in fig. 2, the RF receiver coil subsystem 18 is designed as a multi-element coil, whereby a first coil-like element 19 is fixed to the main  
30 magnet system 15, and whereby a second coil-like element 20 is fixed to the object 14. The first coil-like element 19, which is fixed to the main magnet system 15, is placed directly below the support or bed 17, close to the posterior part of the object 14. The second coil-like element 20, which is fixed to the object 14, is placed on top of the object 14, namely directly on the anterior part of the object 14. For that, the first coil-like element 19 and the second

coil-like element 20 acting together as a receiver coil are positioned close to the object 14 to be analyzed.

Fig. 3 shows a second embodiment of a magnetic resonance imaging device comprising a RF system, namely a RF receiver coil subsystem, according to the present invention. The embodiment according to fig. 3 comprises similar components like the embodiment of fig. 2. For that, in order to avoid unnecessary repetitions, same reference numerals are used.

The embodiment of fig. 3 differs from the embodiment of fig. 2 only with respect to the feature that the first coil-like element 19 of the RF receiver coil subsystem 18 is not fixedly attached to the main magnet system 15, but moveably attached thereto. For that, the support or bed 17 can be moved relative to the first coil-like element 19, and in addition, the first coil-like element 19 can be moved relative to the support or bed 17 on which the object 14 to be analyzed is positioned and relative to the main magnet system 15. Such a configuration can be used to optimize image quality.

In the upper part of fig. 3 pre-scans of the object 14 to be analyzed are obtained at a certain position  $x$  of the support or bed 17. In order to optimize image quality, the bed 17 is slightly moved to the position  $x+\Delta x$  as shown in the middle part of fig. 3. When the bed 17 is moved to the position  $x+\Delta x$ , the second coil-like element 20 of the RF receiver coil subsystem 18 attached to the object 14 on the anterior part of the object 14 moves by the distance  $\Delta x$ . It should be noted that the distance  $\Delta x$  is only a small distance. In case that the image quality at the position  $x+\Delta x$  is better compared to the image quality at the position  $x$  of the bed 17, the first coil-like element 19 of the RF receiver coil-subsystem 18 can be slightly moved by the distance  $\Delta x$  as shown by the arrow 22 in the lower part of fig. 3. By moving the first coil-like element 19 by the distance  $\Delta x$ , the pre-scans are also valid for the bed 17 at the position  $x+\Delta x$ .

Compared to a RF system for which all coils are attached to the object to be analyzed and for which all coils move with the object 14 to be analyzed, there are advantages for the operator of the magnetic resonance imaging device and for the object to be analyzed. For the operator, it is much easier to set up the object to be analyzed because of the fact, that only the second coil-like element 20 has to be attached to the object 14 and that fewer cables have to be connected to the MRI device. For the object 14 to be analyzed, the comfort can be increased, because of the fact, that there are no coils positioned between the bed 17 and the posterior part of the object 14. In addition, there is more space available in the examination

space 16. Compared to a device, where all parts of the RF receiver coil subsystem are fixed to the main magnet system, a higher signal-to-noise ratio can be achieved, because of the fact that the parts of the RF receiver coil subsystem are positioned closer to the object to be analyzed.

5                    In both embodiments shown in Figs. 2 and 3, the second coil-like element 20, which is assigned to the object 14 to be analyzed, can be designed as a wearable unit. Said wearable unit is attachable to the object 14 to be analyzed before MRI analysis outside the magnetic resonance imaging device. So, the object 14 can put on such a wearable unit before the examination starts.

10                   Further on, the bed 17 can be designed in a way that the bed 17 is compatible with a trolley system. This would allow to prepare the object to be analyzed on such a trolley outside an examination room, including the placement of the second coil-like element 20. It is then possible to transport the object 14 to be analyzed to the MRI device already prepared for examination.



## CLAIMS:

1. An RF system for a magnetic resonance imaging device (13), comprising an RF transmitter coil subsystem and an RF receiver coil subsystem (18), characterized in that the RF receiver coil subsystem (18) comprises at least one first coil-like element (19) and at least one second coil-like element (20), wherein the or each first coil-like element (19) is assigned to a main magnet system (15) of the magnetic resonance imaging device (13), and wherein the or each second coil-like element (20) is assigned to an object (14) to be analyzed by the magnetic resonance imaging device (13).
2. An RF system according to claim 1, characterized in that the or each first coil-like element (19) is positioned below, preferably directly below, a support or bed (17) on which the object (14) to be analyzed is placed.
3. An RF system according to claim 2, characterized in that the or each first coil-like element (19) is designed as part of a built-in system body coil.
4. An RF system according to claim 2, characterized in that the or each first coil-like element (19) is attached to the main magnet system (15) of the magnetic resonance imaging device, in a way that a relative movement between said support or bed (17) and the or each first coil-like element (19) is possible.
5. An RF system according to claim 4, characterized in that the or each first coil-like element (19) is fixedly attached to said main magnet system (15), in a way that the support or bed (17) is moveable relative to the or each fixed first coil-like element (19).
6. An RF system according to claim 4, characterized in that the or each first coil-like element (19) is moveably attached to the main magnet system (15), in a way that the support or bed (17) is moveable relative to the or each first coil-like element (19) and that the or each first coil-like element (19) is moveable relative to the main magnet system (15).

7. An RF system according to claim 1, characterized in that the or each second coil-like element (20) is positioned above, preferably directly above, the object (14) to be analyzed by the magnetic resonance imaging device.

5 8. An RF system according to claim 7, characterized in that the or each second coil-like element (20) is attached to the object (14) to be analyzed, in a way that the or each second coil-like element (20) is moveable together with the object (14) to be analyzed.

9. An RF system according to claim 8, characterized in that the or each second  
10 coil-like element (20) is moveable together with a support or bed (17) on which the object (14) to be analyzed is placed relative to the or each first coil-like element (19).

10. An RF system according to claim 7, characterized in that the or each second coil-like element (20) is designed as a wearable unit, wherein said wearable unit is attachable  
15 to the object (14) to be analyzed before MRI analysis outside the magnetic resonance imaging device.

11. A magnetic resonance imaging device (13), comprising a main magnet system (15), a gradient coil system, an RF system and a signal processing system, said RF system  
20 comprising an RF transmitter coil subsystem and an RF receiver coil subsystem (18), characterized in that the RF receiver coil subsystem (18) comprises at least one first coil-like element (19) and at least one second coil-like element (20), wherein the or each first coil-like element (19) is assigned to the main magnet system (15), and wherein the or each second coil-like element (20) is assigned to an object (14) to be analyzed by the magnetic resonance  
25 imaging device (13).

12. A magnetic resonance imaging device (13) according to claim 11, characterized in that the RF system is an RF system according to any one of the preceding claims 2 to 10.

**ABSTRACT:**

The present invention relates to an RF system for a magnetic resonance imaging device (13). The RF system comprises an RF transmitter coil subsystem and an RF receiver coil subsystem (18), wherein the RF receiver coil subsystem comprises at least one first coil-like element (19) and at least one second coil-like element (20), wherein the or each  
5 first coil-like element is assigned to a main magnet system (15) of the magnetic resonance imaging device, and wherein the or each second coil-like element is assigned to an object (14) to be analyzed by the magnetic resonance imaging device.

Fig. 2





1/3

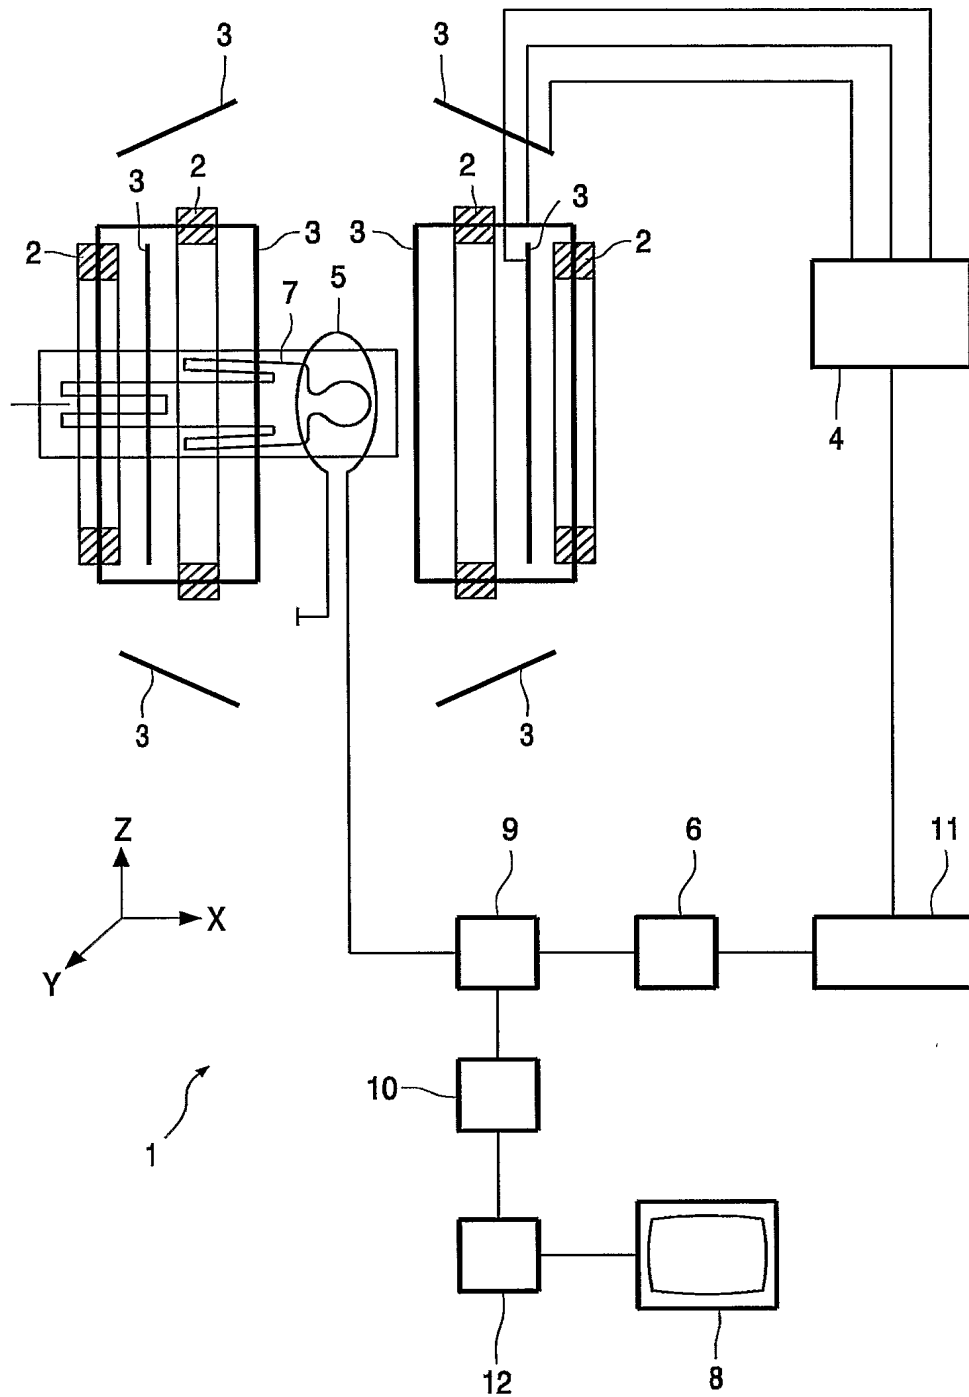


FIG. 1

2/3

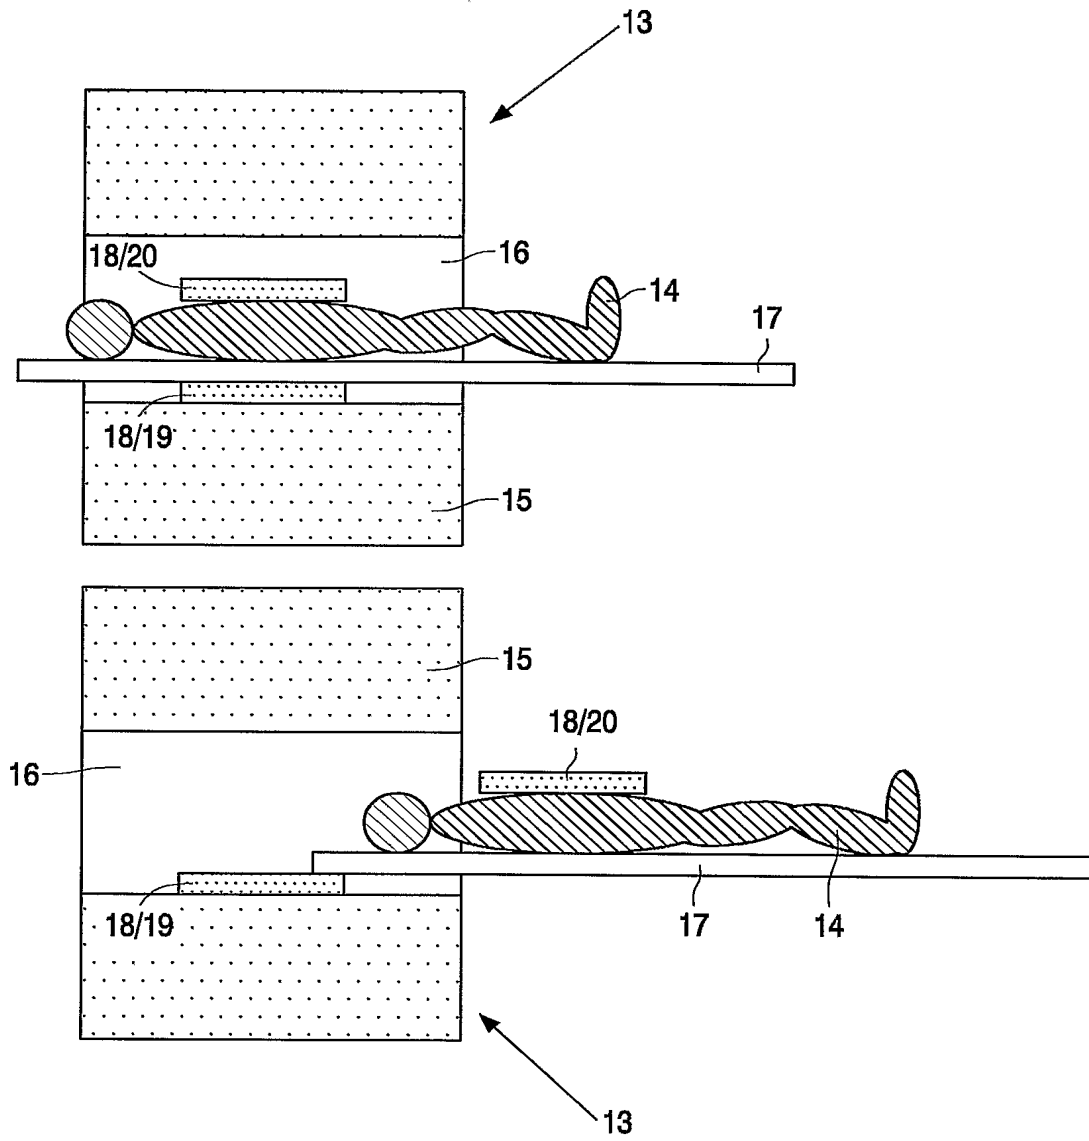


FIG. 2

3/3

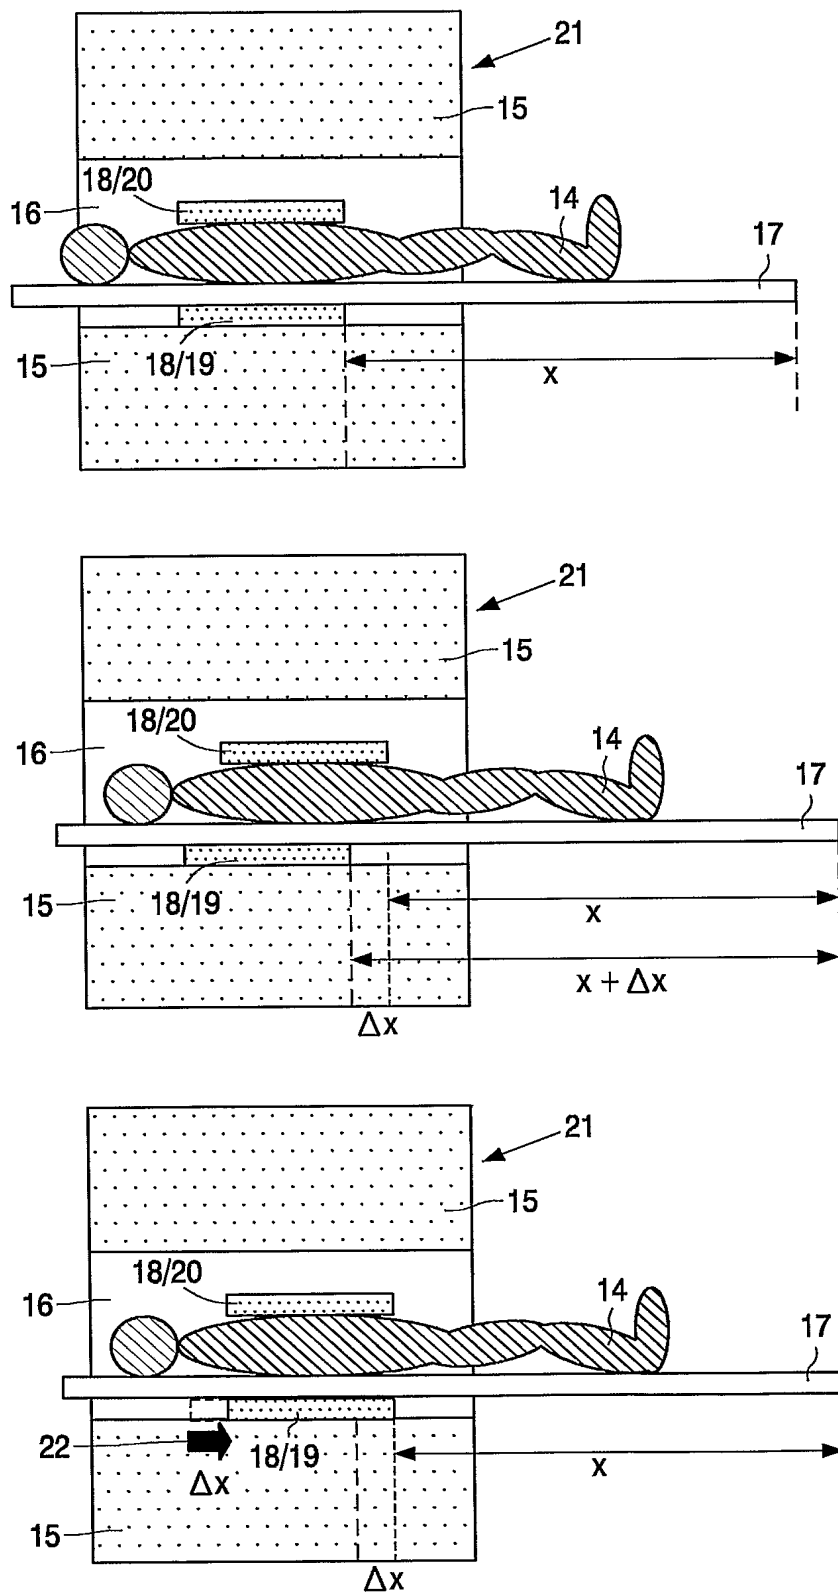


FIG. 3

PCT/IB2005/050447

